


•

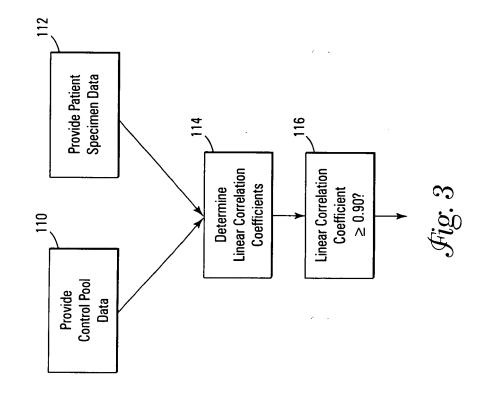

CLICAL ASSAY CALIBRATION ADJUSTMENT METHOD George G. Klee 09/853,867

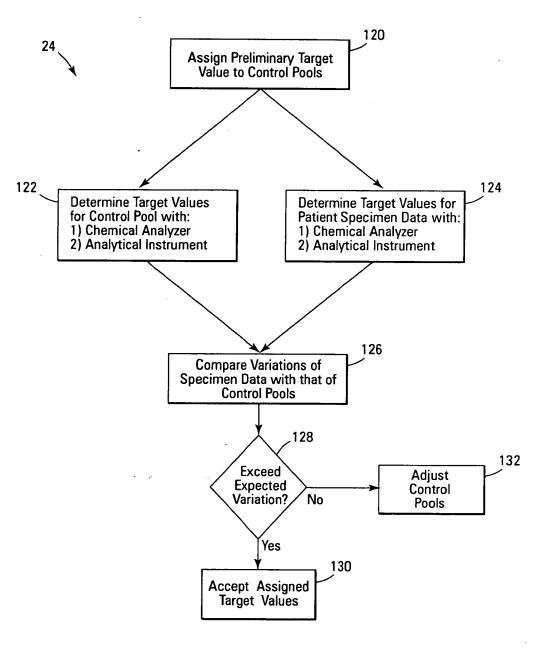
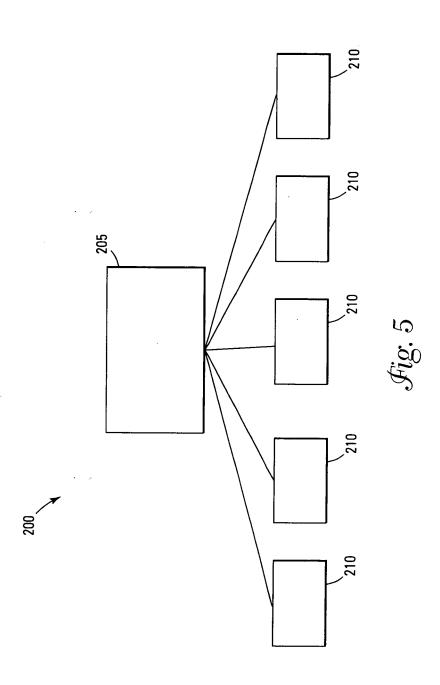
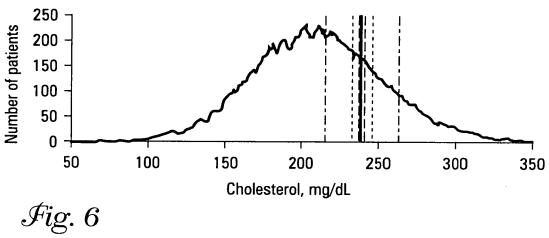


Fig. 4





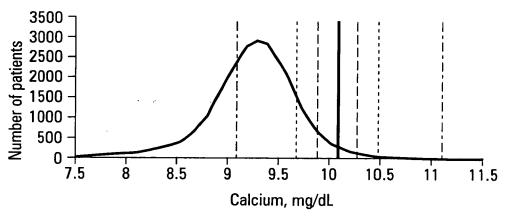
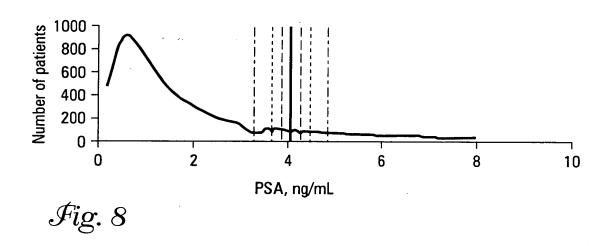
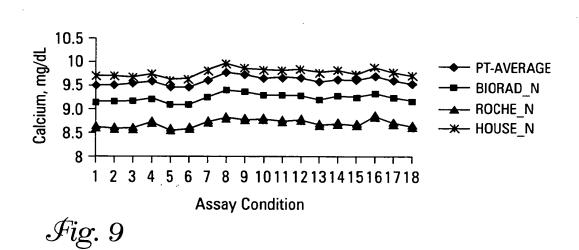


Fig. 7





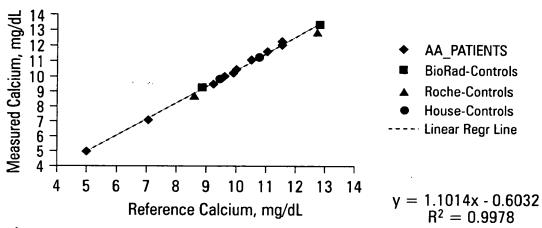


Fig. 10

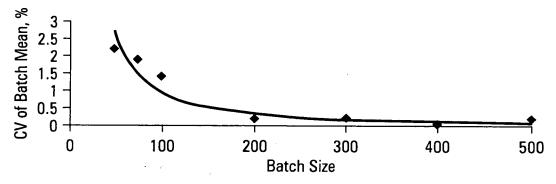


Fig. 11

